

ASIAN CARDIOVASCULAR & THORACIC ANNALS

A Case of 24 Years Longevity of an Ionescu-Shiley Bioprosthesis in the Mitral Position

Yutaka Watanabe, Shuuichi Ohkawa, Keisuke Yamabuki, Hidekazu Tsuneoka, Noboru Sugiyama and Teruo Hiyama
Asian Cardiovasc Thorac Ann 2006;14:96-98

This information is current as of December 2, 2009

The online version of this article, along with updated information and services, is located on the World Wide Web at:

<http://asianannals.ctsnetjournals.org/cgi/content/full/14/5/e96>

The Asian Cardiovascular & Thoracic Annals is the official journal of The Asian Society for Cardiovascular Surgery and affiliated journal of The Association of Thoracic and Cardiovascular Surgeons of Asia.

A Case of 24 Years Longevity of an Ionescu-Shiley Bioprosthesis in the Mitral Position

Yutaka Watanabe, PhD¹, Shuuichi Ohkawa, MD, Keisuke Yamabuki, PhD,
Hidekazu Tsuneoka, MD, Noboru Sugiyama, MD, Teruo Hiyama, PhD

*Department of Cardiovascular Surgery
Higashitoride Hospital
Ibaraki, Japan*

*¹Division of Cardiovascular Surgery
Kiryu Kosei General Hospital
Kiryu, Japan*

ABSTRACT

Valve dysfunction, attributed to primary tissue failure several years after implantation of Ionescu-Shiley bioprostheses, has led to re-operation in most cases. We report a rare case of this bioprosthesis showing stenosis and regurgitation after implantation in the mitral position 24 years previously. No cusp tears, but severe calcification and well-grown neointima over the Dacron cloth of the inner surface were observed. This may explain how the valve functioned for such a long period of time. We replaced it with a Carpentier-Edwards pericardial bioprosthesis.

(Asian Cardiovasc Thorac Ann 2006;14:e96-8)

INTRODUCTION

Initially, the Ionescu-Shiley bioprosthesis (Shiley, Inc., Irvine, CA, USA) was widely used due to clinical characteristics of good hemodynamics with a virtual absence of thromboembolic complications. However, it became clear that re-valve substitution was needed due to malfunction caused mainly by primary tissue failure such as tears and perforations which occurred near the junction of the leaflets and struts. Presumably, in many cases these problems were associated with defects in the structure of the valve. Therefore, the use of Ionescu-Shiley bioprostheses had discontinued by the mid-1980s, and most reports of re-valve substitution disappeared by the end of the 1990s.

CASE REPORT

A 69-year-old male taxi driver, who had undergone implantation of an Ionescu-Shiley bioprosthesis (27 mm) in the mitral position in August 1980 for mitral regurgitation, was hospitalized with severe heart failure. Symptoms of breathlessness on exertion deteriorated from about three months prior to hospitalization, and an expansion of cardio-thoracic ratio was seen. Echocardiography revealed mitral stenosis

(MVA 0.9 cm²), slight mitral regurgitation, and severe tricuspid valve regurgitation. In addition, the left atrial diameter was expanded to 50 mm.

Medical treatment for acute heart failure treatment was initiated, resulting in only minimal improvement. Due to progressive deterioration of the heart failure, mitral valve re-replacement and tricuspid annuloplasty were performed on the 55th day after hospitalization. Via a median sternotomy, a two-staged venous cannula was inserted from the right femoral vein, with the tip located in the superior vena cava (SVC). After right atriotomy and atrioseptostomy, the mitral Ionescu-Shiley bioprosthesis was carefully examined. The annular ring and struts of the bioprosthesis were completely covered with neointima and severe calcification was observed, however no major perforation or tears were noted. Calcification and hardening of the tissue were considered to be the main causes of the severe mitral stenosis and slight regurgitation. The bioprosthesis was carefully removed.

A 25 mm Carpentier-Edwards Perimount pericardial bioprosthesis (Edwards Lifesciences, Inc., CA, USA)

For reprint information contact:

Yutaka Watanabe, PhD Tel: 81 277 44 7171 Fax: 81 277 44 7170 Email: yuwatanabe-ths@umin.ac.jp
Division of Cardiovascular Surgery, Kiryu Kosei General Hospital, Orihime 6-3, Kiryu, Gunma 376-0024, Japan.

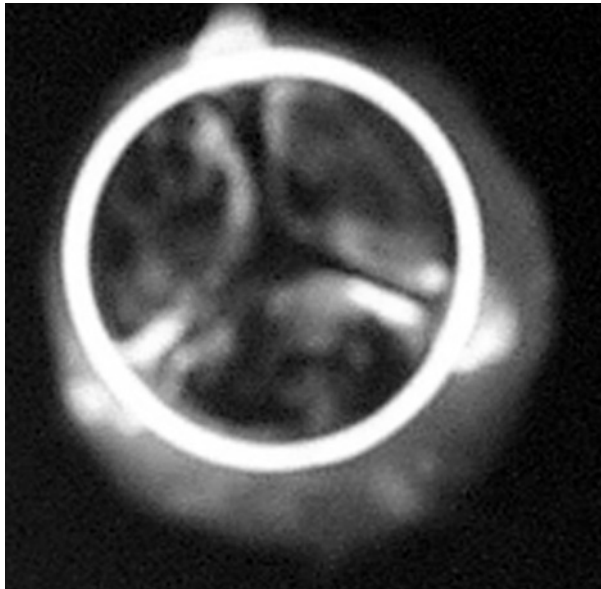


Figure 1. X-Ray examination of the removed valve revealed remarkable calcification observed almost uniformly in all leaflets.

was implanted, and tricuspid annuloplasty was performed using a Cosgrove-Edwards Ring (32 mm diameter) (Edwards Lifesciences, Inc., CA, USA). Postoperative X-Ray examination of the explanted valve revealed almost uniform calcification in all leaflets (Figure 1).

DISCUSSION

The Ionescu-Shiley bioprosthesis was developed by Ionescu in 1971, and marketing was started by Shiley in 1976. Ionescu et al reported malfunction in seven among 336 cases over 10 years of implantation in the mitral position: a low complication rate of 0.6% per patient-year.¹ However in the 1980s, malfunctions especially regurgitation as a result of destruction of leaflets and the resultant hemolysis, were reported within three to five years of use. Consequently the use of Ionescu-Shiley bioprostheses was abandoned. There has been scant mention of Ionescu-Shiley bioprostheses in the international literature subsequent to reports of re-valve substitution by Masters et al (1995), Abe et al (1997), and Machida et al (2001).^{2,3,4} In many reports, the cause of the valve malfunction was attributed to tears and lacerations in the junction of the leaflets, the leaflets themselves, the struts and/or the annular ring of the bioprosthesis.

Gabbay and colleagues reported compelling findings after histologic examination of the excised bioprosthesis. While a mild to moderate degree of disruption in collagen fibers existed in the torn part of leaflet, there was neither severe calcification nor infection. Moreover, neointimal formation was not evident on the Dacron cloth of the ring and struts. Destruction of the leaflet

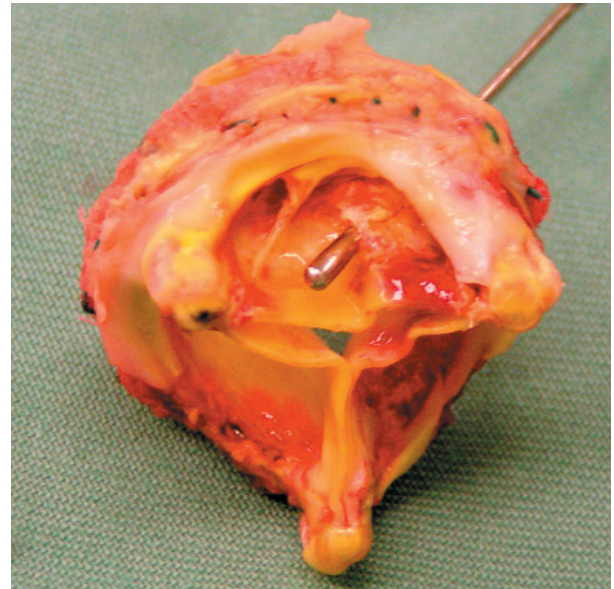


Figure 2. Photograph showing a very small perforation in the center of the leaflet indicated by the metallic probe; the ring and struts are well covered with neointima, and severe calcification is evident.

may have occurred as a result of mechanical factors; such as friction or fatigue within the struts and leaflets, which lacked the neointima.^{5,6}

Schoen et al reported cuspal calcification and defects clearly associated with commissural sutures ("alignment stitches") unique to this valve design. Additionally, gross cuspal thickening and mild stretching and microscopic deep fluid insudation, separation of collagen bundles, and mononuclear inflammation were observed within 7 years postoperatively.⁷

In our case, most portions of the Dacron cloth were covered with well-grown neointima, which might decrease physical stress on the leaflets and be a main reason why the valve functioned over a long period of time without tears or major perforation of the leaflets. We examined the removed valve in detail and found a small perforation, which was not identified during the operation, and very severe calcification and hardening of all the leaflets but no infected vegetation (Figure 2). Such severe calcification is inevitable over a 24-year period due to inherent bio-reaction processes.

We conclude that these findings support the hypotheses of Gabbay et al⁶. It is evident that the design, the materials including chemical fixation, and the technical fabrication are all critical aspects of prosthetic valve development. In addition, this case appears to be the only reported incidence of a prosthetic valve functioning in excess of 20 years, as the mean time to re-operation of most bioprostheses is 11.5 ± 7.1 years.⁸

REFERENCES

1. Ionescu MI, Smith DR, Hasan SS, Chidambaram M, Tandon AP. Clinical durability of the pericardial xenograft valve: ten years experience with mitral replacement. *Ann Thorac Surg* 1982;34:265–77.
2. Masters RG, Walley VM, Pipe AL, Keon WJ. Long-term experience with the Ionescu-Shiley pericardial valve. *Ann Thorac Surg* 1995;60(2 Suppl): S288–91.
3. Abe M, Sakai A, Hanayama N, Lin ZB, Oosawa M. Reoperation for malfunction of Ionescu-Shiley bovine pericardial bioprosthetic valves in the mitral position--special consideration with emergency operation. *Nippon Kyobu Geka Gakkai Zasshi* 1997;45:17–22.
4. Machida H, Ishibashi-Ueda H, Nakano K, Sasako Y, Kobayashi J, Bando K, et al. A morphologic study of Carpentier-Edwards pericardial xenografts in the mitral position exhibiting primary tissue failure in adults in comparison with Ionescu-Shiley pericardial xenografts. *J Thorac Cardiovasc Surg* 2001;122:649–55.
5. Gabbay S, Bortolotti U, Wasserman F, Factor S, Strom J, Frater RW. Fatigue-induced failure of the Ionescu-Shiley pericardial xenograft in the mitral position. In vivo and in vitro correlation and a proposed classification. *J Thorac Cardiovasc Surg* 1984;87:836–44.
6. Gabbay S, Bortolotti U, Wasserman F, Tindel N, Factor SM, Frater RW. Long-term follow-up of the Ionescu-Shiley mitral pericardial xenograft. *J Thorac Cardiovasc Surg* 1984;88(5 Pt 1):758–63.
7. Schoen FJ, Fernandez J, Gonzalez-Lavin L, Cernaianu A. Causes of failure and pathologic findings in surgically removed Ionescu-Shiley standard bovine pericardial heart valve bioprostheses: emphasis on progressive structural deterioration. *Circulation* 1987;76:618–27.
8. Potter DD, Sundt TM 3rd, Zehr KJ, Dearani JA, Daly RC, Mullany CJ, et al. Risk of repeat mitral valve replacement for failed mitral valve prostheses. *Ann Thorac Surg* 2004;78:67–72.

A Case of 24 Years Longevity of an Ionescu-Shiley Bioprosthesis in the Mitral Position

Yutaka Watanabe, Shuuichi Ohkawa, Keisuke Yamabuki, Hidekazu Tsuneoka, Noboru Sugiyama and Teruo Hiyama

Asian Cardiovasc Thorac Ann 2006;14:96-98

This information is current as of December 2, 2009

Updated Information & Services	including high-resolution figures, can be found at: http://asianannals.ctsnetjournals.org/cgi/content/full/14/5/e96
References	This article cites 8 articles, 6 of which you can access for free at: http://asianannals.ctsnetjournals.org/cgi/content/full/14/5/e96#BIBL
Subspecialty Collections	This article, along with others on similar topics, appears in the following collection(s): Valve disease http://asianannals.ctsnetjournals.org/cgi/collection/valve_disease
Permissions & Licensing	Requests to reproduce this article in parts (figures, tables) or in its entirety should be submitted via email to: info@asiapex.com
Reprints	For ordering reprints, please email: info@asiapex.com

